

# Kreatech™ FISH probes

## Product Information Sheet

KI-10117


6q21 / MYC (8q24)

100 µl

**DANGER**



**FORMAMIDE**





**Kreatech Biotechnology B.V.**  
Vlierweg 20  
1032 LG Amsterdam  
The Netherlands  
[www.LeicaBiosystems.com](http://www.LeicaBiosystems.com)

**RUO - Research Use Only**

Not for use in diagnostic procedures

PI-KI-10117\_D2.1

Published August 2015

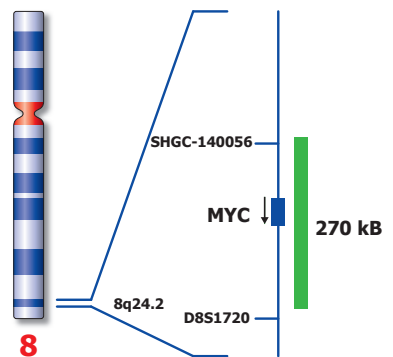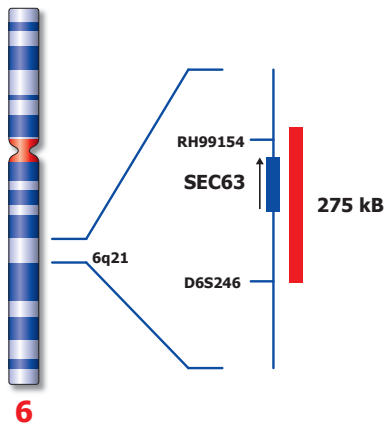

Not to scale

KI-10117

## Kreatech™ 6q21 / MYC (8q24) FISH probe

**Introduction:** The **6q21** specific FISH probe is optimized to detect 6q at 6q21. The **MYC (8q24)** FISH probe is optimized to detect the MYC gene region at 8q24.

**Critical region 1 (red):** The **6q21** specific FISH probe is direct-labeled with PlatinumBright™550.  
**Critical region 2 (green):** The **MYC (8q24)** specific FISH probe is direct-labeled with PlatinumBright™495.

**Reagent:** Kreatech probes are direct-labeled DNA probes provided in a ready-to-use format. Apply 10 µl of probe to a sample area of approximately 22 x 22 mm.

**Please refer to the Instructions for Use for the entire Kreatech FISH protocol.**

**Kreatech FISH probes are REPEAT-FREE™ and therefore do not contain Cot-1 DNA. Hybridization efficiency is increased and background, due to unspecific binding, is highly reduced.**

**Patterns:** The **6q21 / MYC (8q24)** FISH probe is designed as a dual-color assay to detect deletions and amplifications at 6q21 and 8q24. Deletions involving the 6q21 region will show one red signal and two green signals for the MYC region at 8q24 (1R2G). Amplifications involving the MYC gene region will show three or more green signals and two red signals for the 6q21 region (2R3+G). Deletions and Amplifications involving both critical regions at 6q21 and 8q24 will show one red and three or more green signals (1R3+G). Two single color red (R) and green (G) signals will identify the normal chromosomes 6 and 8 (2R2G).

	Normal Signal Pattern	Del(6q21)	Amp (8q24)
Expected Signals	2R2G	1R2G	2R3+G

**References:** Zhang, Y, 2000, Genes, Chrom. And Canc. 27; 52-58  
Bentz, M et al, 1995, Blood, 85; 3610-3618

**Warning and precautions:** In case of emergencies check SDS sheets for medical advice. SDS sheets may be obtained by either contacting Leica Technical Support or visiting [www.LeicaBiosystems.com](http://www.LeicaBiosystems.com). DNA probes contain formamide which is a teratogen; do not inhale or allow skin contact. Wear gloves and a lab coat when handling DNA probes. All materials should be disposed of according to your institution's guidelines for hospital waste disposal.

**Reagent Storage and Handling:** Store at 2-8 °C. Reagents should not be used after the expiration date on the vial label.

**TECHNICAL SUPPORT** Technical support is available at [www.LeicaBiosystems.com/service-support/technical-support/](http://www.LeicaBiosystems.com/service-support/technical-support/) or toll free at 800-248-0123 or via e-mail: [kreatech-support@leicabiosystems.com](mailto:kreatech-support@leicabiosystems.com).

**CUSTOMER SERVICE** Kreatech probes may be ordered through Leica Customer Service toll free at 800-248-0123 or order via e-mail: [purchase\\_orders@leica-microsystems.com](mailto:purchase_orders@leica-microsystems.com).